


Certificate of Analysis

GHK Copper 50mg, BPC-157 10mg, Thymosin beta4 10mg

Compound : GHK-Cu, BPC-157, Thymosin beta4 **Client** : AIO Peptides
Lot number : CG-95 AIOPeptides.com
Analysis date : 2025-06-02 Hello@AIOPeptides.com
Purity % : 99.66%
Method : HPLC-UV-MS

High Performance Liquid Chromatography (HPLC) UV – Purity Test

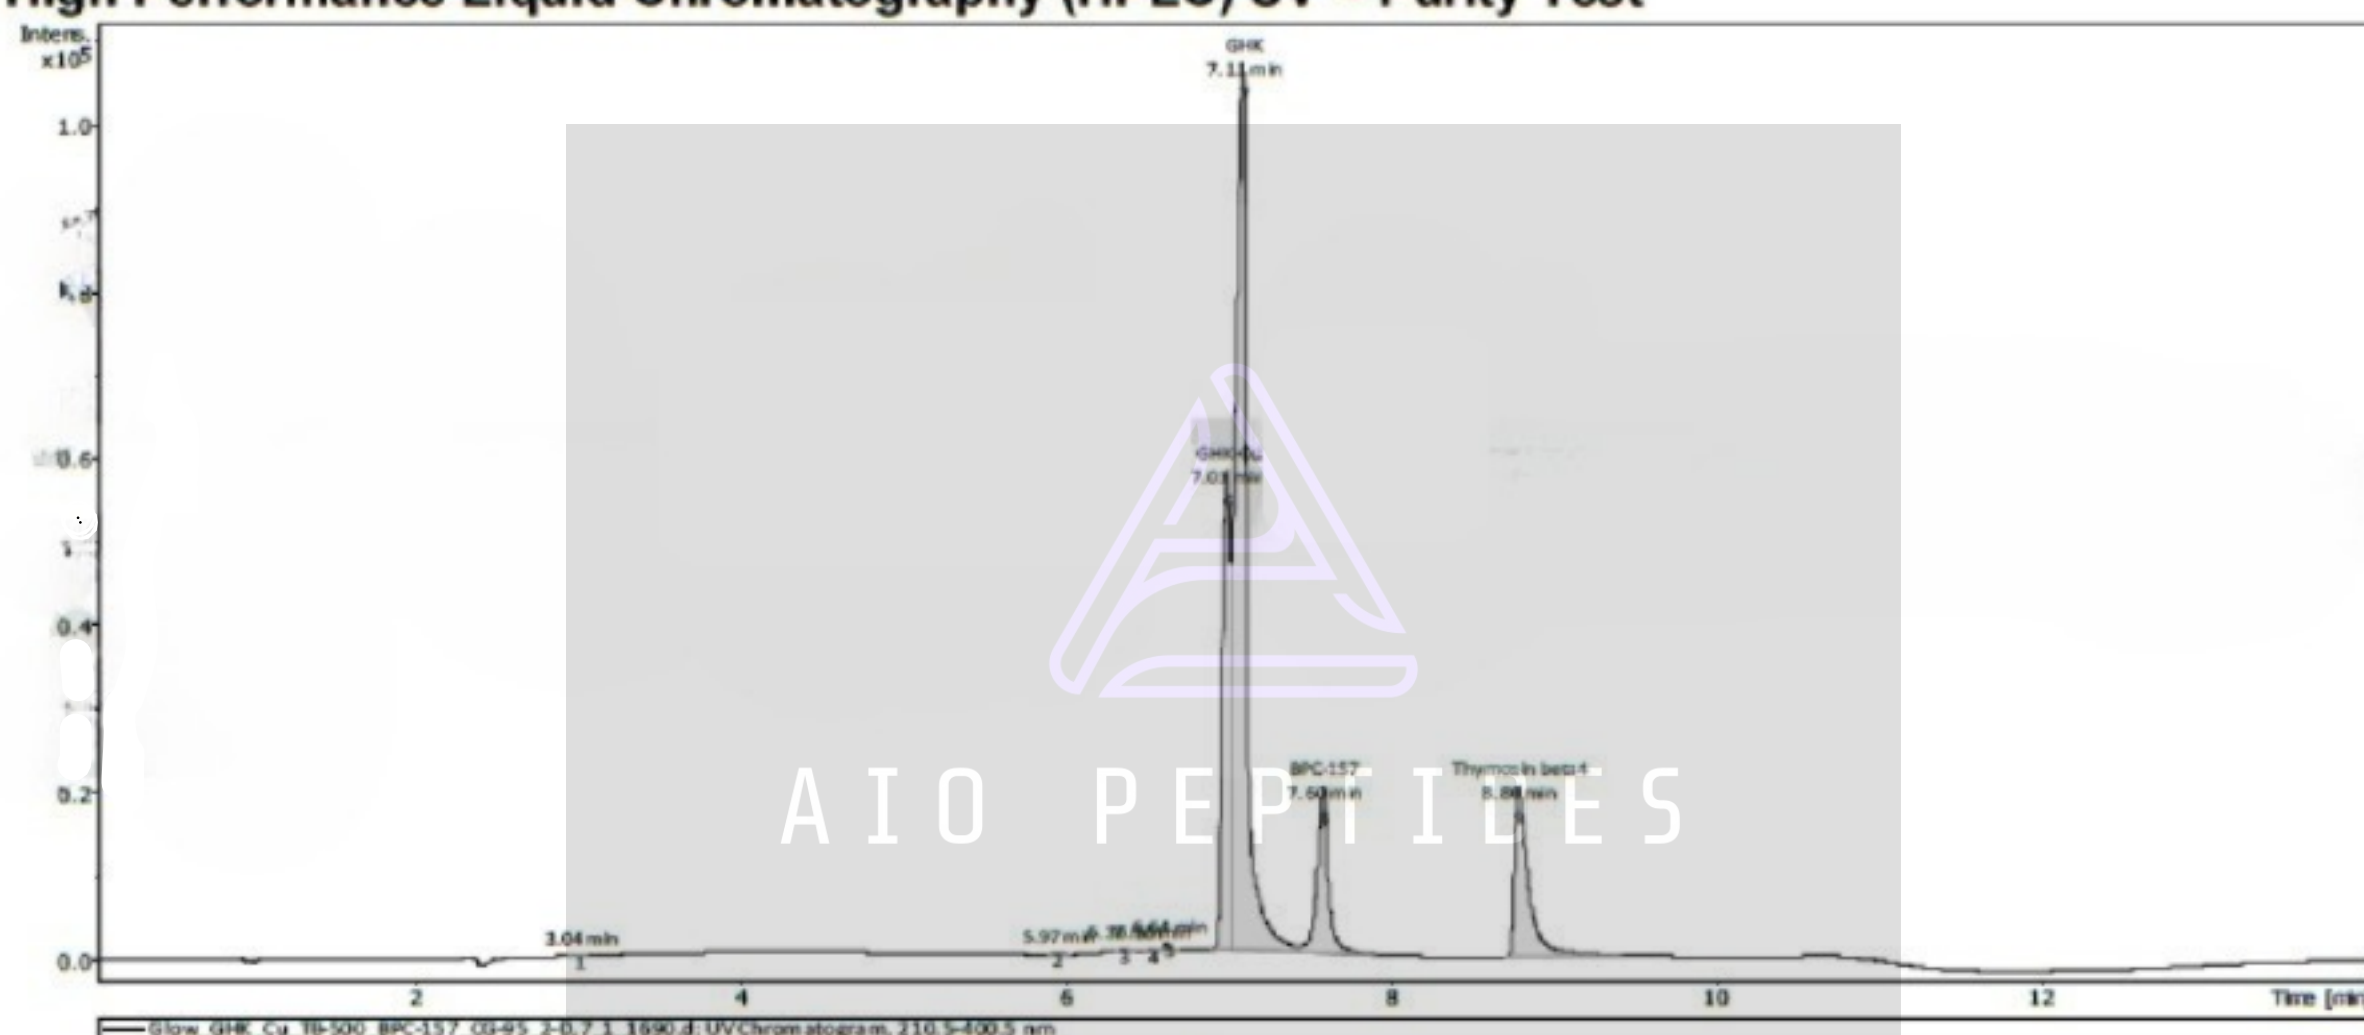


PEAK LIST		Number of detected peaks: 9		
	Time (min)	Area	%Area	
1	3.04	1.47E+02	0.02	
2	5.97	5.85E+02	0.06	
3	6.37	5.78E+02	0.06	
4	6.55	1.53E+02	0.02	
5	6.64	1.67E+03	0.18	
6	7.01	1.94E+05	20.55	GHK-Cu
7	7.11	5.29E+05	56.04	GHK
8	7.60	9.71E+04	10.28	BPC-157
9	8.80	1.21E+05	12.79	Thymosin beta4

Overall Purity : 99.66

The overall purity is good.
But copper concentration in GHK-Cu complex is low
because GHK peak is bigger than the GHK-Cu complex.

Note: Injectable peptides may contain salts and sugars to aid in solubility and act as pH buffers.
These are not normally detected using UV and are not considered impurities.

Analysis Performed by
Ken Pendarvis, ChE
Analytical Chemist
MZ Biolabs
contact@mzbiolabs.com

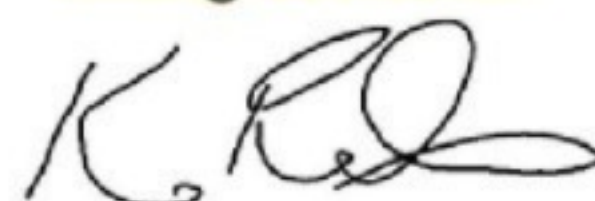

2025-06-03